LOUDSPEAKER AMPLIFIER
TYPE 4062/02
(Part No. 844062/02)

INSTRUCTION AND MAINTENANCE MANUAL

Supplied for use with
Equipment Serial No(s) .....

Made on Order No. 19/5088

Customer's Order No. 3170

UAG

PYE T.V.T. LTD
CAMBRIDGE
ENGLAND

PUBLICATION 1953
B.B.C.

This page is blank to preserve page binding order on printing

C O N T E N T S

	Page
SECTION 1 - INTRODUCTION	1
SECTION 2 - SPECIFICATION	3
SECTION 3 - INSTALLATION AND OPERATION	
3.1 Preparation	5
3.2 Insertion	5
3.3 Controls	5
SECTION 4 - TECHNICAL DESCRIPTION	
4.1 Input Stages	7
4.2 Power Output Stages	7
4.3 Power Supplies	8
4.4 Rating and Cooling	8
SECTION 5 - MAINTENANCE AND FAULT FINDING	
5.1 Access to Components	9
5.2 Voltage and Current Analysis	9
5.3 Resistance of Windings	10
5.3.1 High Permeability Cored Transformers	11
SECTION 6 - PARTS LIST	
6.1 Resistors	13
6.2 Capacitors	13
6.3 Semiconductors	13
6.4 Transformers	14
6.5 Miscellaneous	14
APPENDICES	
1 Unit Mounting and Wiring Techniques	
2 Maintenance Precautions on Semiconductor Units	
3 Demagnetisation of High Permeability Cores	
DIAGRAM	
Circuit Diagram	Following Page 6

Broadcast Television Technology Trust -- bttt.org.uk

This page is blank to preserve page binding order on printing

SECTION 1 - INTRODUCTION

This unit is of unusual design, and has a technical performance of an exceptionally high standard.

The amplifier has a low distortion level and may be used as a high quality audio monitor in a situation where a high acoustic output is not required.

Two separate inputs are provided, these allow mixing of signals from two sources.

The power supply is an integral part of the unit, but provision is made for an external d.c. supply to be connected when necessary.

Two versions of this unit are supplied; on one version the a.c. switch is up for 'ON', whilst on the alternative version the switch is down for 'ON'.

This page is blank to preserve page binding order on printing

SECTION 2 - SPECIFICATION

Input Impedance (Measured at 60 c/s, 1 kc/s and 8 kc/s)	
(each input)	Greater than 10k ohms ± j 20%
Input Isolation	
(each input)	Greater than 50 dB
Gain (both inputs)	29 dB ± 1 dB
Frequency Response	(relative to 1 kc/s)
	30 c/s to 15 kc/s ± 1 dB 60 c/s to 8 kc/s ± 0·2 dB
Distortion (measured at 30 c/s, 1 kc/s and 8 kc/s: 2 watts output)	
	Less than 1%
Noise (both inputs)	
	Less than -60 dBm measured at output
Power Supplies	
	85-125V or 170-250V. 47-70 c/s
Supply Requirements	
	20 VA at 2 watts output 16 VA under quiescent conditions

Overall Approximate Dimensions

Height	$5\frac{3}{4}$ in.	($14\frac{1}{2}$ cm)
Width	3 in.	($7\frac{1}{2}$ cm)
Depth	$9\frac{1}{4}$ in.	($23\frac{1}{2}$ cm)

Approximate Weight

5 lb 14 oz. ($2\frac{3}{4}$ kg)

This page is blank to preserve page binding order on printing

SECTION 3 - INSTALLATION AND OPERATION

3.1 PREPARATION

If the unit is to be used as an addition to an existing installation:

(a) Fix the receptacle plate (plus any additional screens which may be necessary), and wire the connector as instructed in the appendix 'Unit Mounting and Wiring Techniques'.

(b) If the internal power supply is to be used:

(i) connect together pins 5 and 13 on the mating connector.

(ii) Insert the voltage selector plug into the correct voltage tapping at the primary of the mains transformer.

(c) If an external power supply is to be used, connect the supply to pins 13 and 15 on the mating connector as indicated on the circuit diagram.

(d) When a group of amplifiers is to be used, forced cooling is advisable.

(e) Check that the fuses are secure.

(f) Always switch off the a.c. supplies before inserting the unit.

3.2 INSERTION

To insert, grasp the handle, and slide the unit into the frame until the catch engages, slightly pull the unit to ensure it is locked into position.

If it becomes necessary to remove the unit, grasp the handle so as to lift up the small catch, the unit may then be pulled out.

For explanations of certain points in the foregoing see the appendix 'Maintenance Precautions on Semiconductor Units'.

3.3 CONTROLS

A 'Gain' control is provided on each input. The dial of each control is calibrated from 0 to 10, the calibration allowing easy resetting if the position is noted.

An a/c mains ON/OFF switch also is provided.

This page is blank to preserve page binding order on printing

SECTION 4 - TECHNICAL DESCRIPTION

4.1 INPUT STAGES

Two separate inputs, each with its separate input transformer, are provided.

The signal enters the first stage via the relative input transformer T1 or T2, and the gain control R2 (R9). A high impedance input is maintained by the resistor R1 (R8) being placed in series with R2 (R9).

From the gain control the signal passes via the isolating capacitor C1 (C4) to the base of VT1 (VT2) which is arranged as a common emitter stage, with the base d.c. potential stabilised by the potential divider R3 and R4 (R10 and R11). These components plus R6 and R7 (R13 and R14) and R15 provide the necessary bias stabilisation. A small amount of feedback is achieved by partially decoupling the emitter stabilising resistor R6 (R13) by C3 (C6).

The signal passes from the collector of VT1 (VT2) via the decoupling capacitor C2 (C5) to the base of VT3, a common emitter stage. Emitter d.c. stabilisation is effected by the voltage developed across R19 and R20. This bias voltage opposes any d.c. change in collector current, and stabilises the d.c. conditions for the stage over a wide range of temperature changes.

VT4 and VT5 are a pair of phase-splitting transistors arranged in a common emitter-common base configuration. The capacitor C10 corrects any tendency for the unterminated amplifier to oscillate.

The B- supply is decoupled between the input and output stages by R28 and C11.

4.2 POWER OUTPUT STAGE

The power amplifier output stage comprises two pairs of transistors in a class A, split load, push-pull arrangement. The circuit may be considered as a super-alpha, common emitter stage.

In the driver stage the potential divider R29, R30, R31 and R32 provides base bias, the emitter stabilisation being effected by R33 and R34.

An unusual feature of the output stage is the provision of local negative feedback to the emitters of the four transistors in the output stage by an additional winding on the primary of the output transformer T3.

Negative feedback derived from the secondary of T3 is applied to the emitter of VT3 and the base of VT4, the network R38 and C16 across R36 in the feedback loop correcting any rising high frequency response.

Feedback applied by the methods used in the amplifier provides enhanced stability coupled with a low distortion content.

R35 limits the maximum dissipation of the output stage.

4.3 POWER SUPPLY

The power supply is an integral part of the unit, but provision is made for the use, when necessary, of power from an outside source. Details for the connection of outside power are given in Section 3 of this book.

Operation of SWA applies a.c. to the selected voltage tapping at the primary of the mains transformer T4.

The d.c. output is derived from the centre tapped secondary winding of T4 via the full wave rectifier MR1 and MR2, giving an unstabilised supply of nominally 16V smoothed by C17. LP1 lights to indicate that a d.c. supply is available.

4.4 RATING AND COOLING

All components, including semiconductors, are operated well within their maximum ratings. Extreme ambient temperatures have been considered and a wide temperature range is acceptable to the unit. Cooling of the power transistors is assisted by the heat dissipation coefficient of the heat sink, and the unit is cooled as a whole by convection in the surrounding air. In this connection attention is drawn to the appendix 'Maintenance Precautions on Semiconductor Units'.

SECTION 5 - MAINTENANCE AND FAULT FINDING

WARNING: Before commencing any checking, fault finding or other maintenance work see the appendix "Maintenance Precautions on Semiconductor Units".

5.1 ACCESS TO COMPONENTS

To obtain access to components inside the unit:

Unscrew the knurled post at the rear of the unit. Remove the screw at the front end of the umpled member which held the knurled post. Loosen the screws at the front and rear of the member at the base of the unit and carefully hinge out the side of the unit on to some flat surface so as **not** to strain the cableform.

5.2 VOLTAGE AND CURRENT ANALYSIS

The location of faults will be facilitated by making checks at the points indicated in the analysis table which follows. The figures given are those measured on a typical unit and measured figures may be found to vary slightly from one unit to another. Deviations from the figures given are not necessarily indicative of faults, but if the supply voltage is set to within ±1V any wide divergency should be investigated.

Conditions

All voltage readings on this unit have been taken with respect to the positive rail, under no signal conditions and on the range quoted, a meter having a sensitivity of 20000 ohms per volt being used.

Abbreviations used in the table:

e = emitter b = base c = collector

Circuit	Location	Meter Range Volts	Measurement Volts
VT1 and VT2	e	2.5	0.4
	b	2.5	0.5
	c	10	3.3
VT3	e	10	1.6
	b	10	1.8
	c	10	4.5

Circuit	Location	Meter Range Volts	Measurement Volts
VT4 and VT5	e	10	2.1
	b	10	2.3
	c	10	7.1
VT6	e	2·5	0·25
	b	2·5	0·4
	c	25	14·5
VT7	e	2·5	0·25
	b	2·5	0·4
	c	25	14·5
VT8	e	2·5	0·1
	b	2·5	0·25
	c	25	14·5
VT9	e	2·5	0·1
	b	2·5	0·25
	c	25	14·5
V_{B-}	C17	25	16
I_{B-}	across FS3	1A d.c.	340 mA

5.3 RESISTANCE OF WINDINGS

NOTE: ALL VALUES ARE ±10%

Transformer T3

Pins	1 - 2	0·38	ohms
"	6 - 7	0·203	"
"	3 - 5	0·017	"
"	9 - 10	0·520	"

Transformer T4

Pins	11 - 13	1·38	ohms
"	1 - 5	73· 4	"
"	6 - 10	80· 5	"

5.3.1 High Permeability Cored Transformers

WARNING:

D.C. Resistance measuring devices and continuity checking equipment, e.g. Avometers should not be used for checking the resistance or continuity of certain transformer windings. The reason for this, and the treatment to be applied if d.c. is accidently used, are dealt with in the appendix 'Demagnetisation of High Permeability Cores' bound in with this manual.

The transformer(s) to which this warning applies are listed below, together with the inductance of the windings and the voltage and frequency at which it is measured, the r.m.s. demagnetising voltage, and the pins to which this voltage is applied.

Circuit Ref.	Inductance/Voltage/Frequency			Demagnetising Volts	Pins
T1 and T2 primary	300H	0·2	50 c/s	33V	1 - 3


This page is blank to preserve page binding order on printing

PARTS LIST
FOR
LOUDSPEAKER AMPLIFIER
TYPE 4062/02

Item				Pye Part No.	Manufacturer	Type
6.1 RESISTORS						
5.1 ohms	±5%	6W		PE05157	Painton	302A
56 ohms	-5%	½W		PE56067	Electrosil	CJ20
82	"	"	½W	PE82067	Dubilier	B.T.T.
180	"	"	"	PE18167	"	"
470	"	±5%	½W	PE47167	"	"
330	"	"	"	PE33167	"	"
390	"	"	"	PE39167	"	"
560	"	"	"	PE56167	"	"
1.2k	"	"	"	PE12267	"	"
1.5k	"	"	"	PE15267	"	"
2.2k	"	"	"	PE22267	"	"
2.7k	"	"	"	PE27267	"	"
3.9k	"	"	"	PE39267	"	"
4.7k	"	"	"	PE47267	"	"
5.6k	"	"	"	PE56267	"	"
6.8k	"	"	"	PE68267	"	"
8.2k	"	"	"	PE82267	"	"
10k	"	"	"	PE10367	"	"
18k	"	"	"	PE18367	"	"
33k	"	"	"	PE33367	"	"
68k	"	"	"	PE68367	"	"
33k	Linear Pot.		2W	PL04219	"	"
6.2 CAPACITORS						
1000pF	±10%	400V		PR01008	Maycon	Wima Tropyfol F
400µF	-10+50%	6.4V		PS44000	Mullard	C426AM/C400
100	"	6.4V		PS40007	"	C426AM/C100
100	"	16V		PS38003	"	C426AM/E100
160	"	10V		PS39200	"	C426AM/D160
400	"	6.4V		PS44000	"	C426AM/C400
1000	"	15V		PS51026	"	CE 1302
5000	"	25V		PS59004	"	1258/8
6.3 SEMICONDUCTORS						
Transistor				FV07000	G.E.C.	GET880
"				FV05010	Mullard	OC24
Diode				FR00019	G.E.C.	SX638

Item	Pye Part No.	Manufacturer	Type
6.4 TRANSFORMERS			
Input	772245	Pye	B8970
Output	772204	"	B8876
Mains	AL20019	"	B9121
6.5 MISCELLANEOUS			
Lamp 28V 1·1W	FL01021	Atlas	S6/8
Plug 16-way	724101	Amphenol	26/159/16
Socket 16-way	724153	"	26/190/16
Lampholder	FL01013	Bulgin	D737/INS/WHITE
Switch D.P.D.T.	830124	N.S.F.	8373/K6
Knob (control)	551403	A.E.I.	2285/17
Voltage Selector Plate	FS16500	McMurdo	B279002
Fuse 500 mA cartridge	701414	Bulgin	PAK2
" 2A "	722371	"	F128

Broadcast Television Technology Trust -- bttt.org.uk

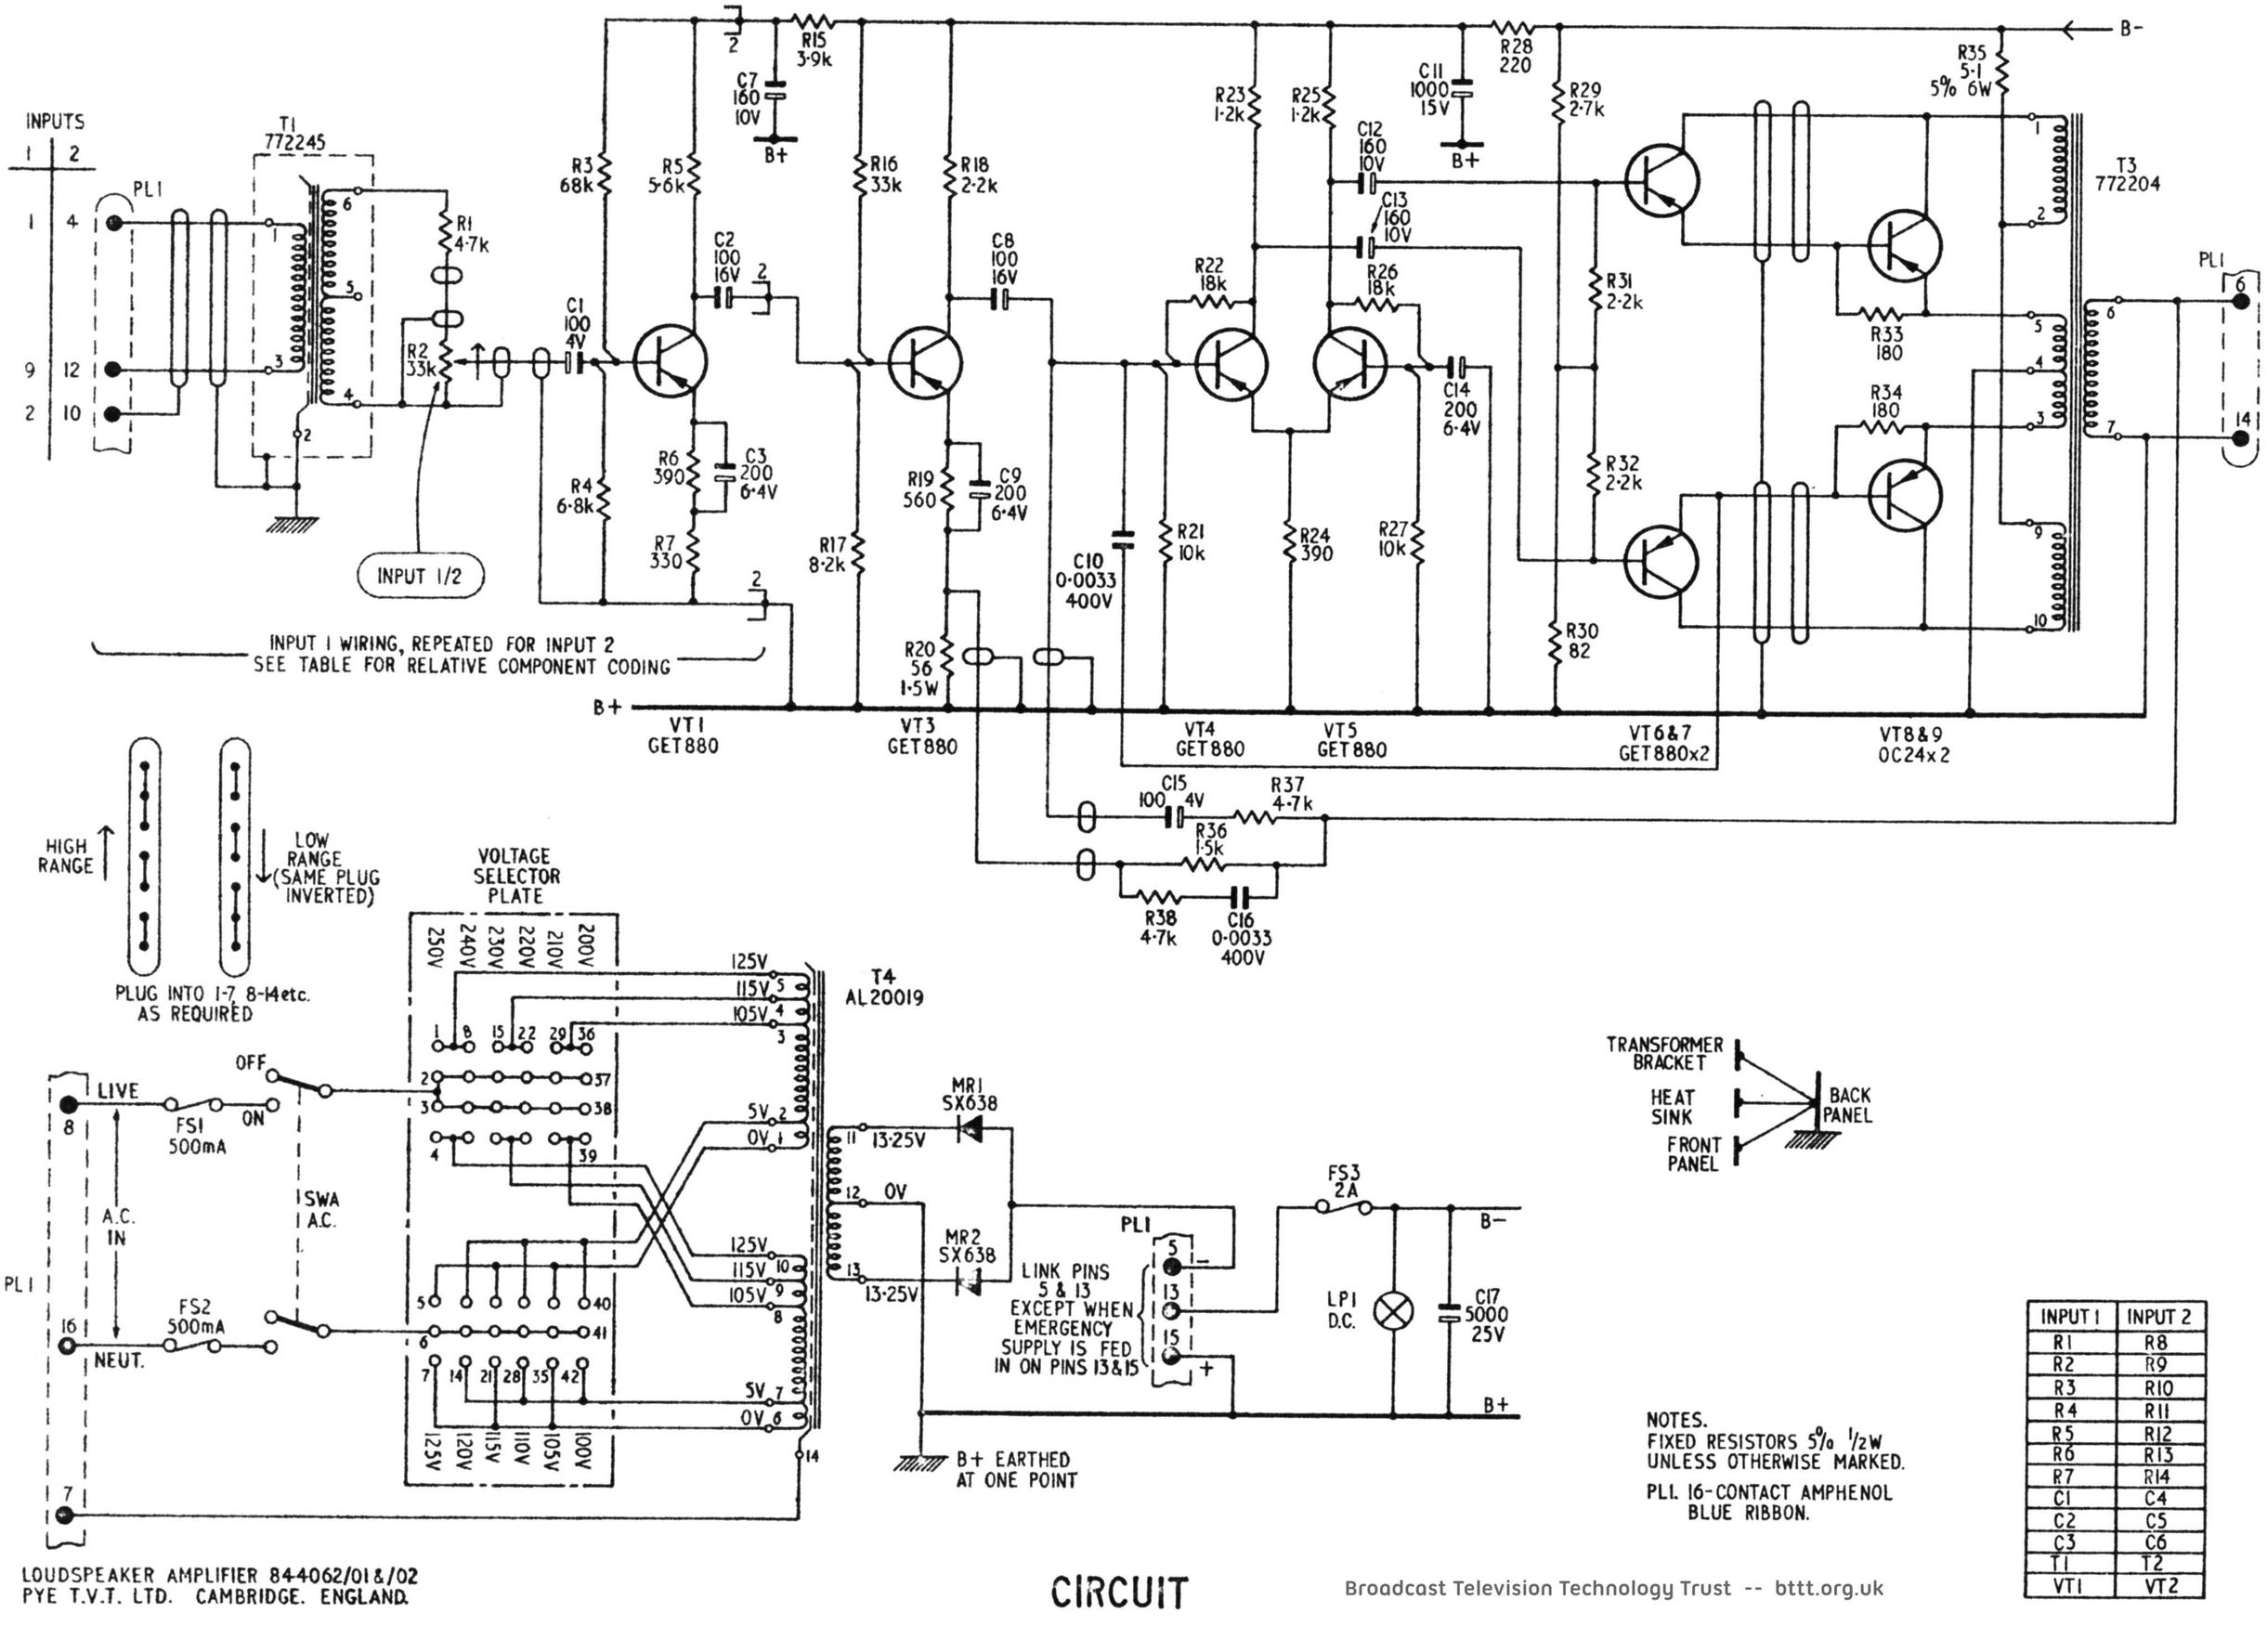

NOTES.
FIXED RESISTORS 5% 1/2W UNLESS OTHERWISE MARKED.

PL1. 16-CONTACT AMPHENOL BLUE RIBBON.

INPUT 1	INPUT 2
R1	R8
R2	R9
R3	R10
R4	R11
R5	R12
R6	R13
R7	R14
C1	C4
C2	C5
C3	C6
T1	T2
VT1	VT2

LOUDSPEAKER AMPLIFIER 844062/01&/02
PYE T.V.T. LTD. CAMBRIDGE. ENGLAND.

CIRCUIT

ISSUE 1

Broadcast Television Technology Trust -- bttt.org.uk

UNIT MOUNTING AND WIRING TECHNIQUES

1. GENERAL

Plug-in units are housed in special frames which can accept different sizes of units (in mixed sizes) and can also provide individual unit screening facilities.

2. FIXING THE FRAME

Some frames are supplied permanently fixed into consoles, others are loose items for bolting into racks. When fixing the frame into any rack observe the following:

(a) Use the fibre washers (supplied with the fixing screws) so as to protect the paint on the front member of the frame.

(b) Do not obstruct the ventilation holes in the top and bottom plates of the frame.

(c) Units generating large amounts of heat should not be positioned immediately beneath the frame.

3. FIXING THE SCREENS

The types of screening plates available can fit into the frame so as to divide it vertically and horizontally as required, i.e. to give a mixture of compartment sizes. Fit these as follows:

(a) Insert vertical screens first by dropping the lugs into the slots provided in the frame and then by slightly bowing the screen allow the other lugs to spring into the opposite slots.

(b) Insert the horizontal screens in the same manner but with the lugs entering the slots in the vertical screens.

4. RECEPTACLE PLATE ASSEMBLY

When units are supplied to fit into the frame a back plate (appropriate to the size of the compartment) is supplied loose. This is complete with fixings and with the unit mating connector already in position. When fitting the plate observe the following:

(a) Ensure that the plate is mounted so as to give the correct pin alignment of the mating connector.

(b) Do not tighten the mating connector fixings; "floating" is deliberate to ensure easy alignment of the unit connector and the mating component.

5. WIRING CONNECTORS

WARNING If the particular unit being installed contains semi-conductors it should not be plugged in during the soldering operation. Similarly other units already in the equipment should be

unplugged if these contain semiconductors, but see the section entitled "Maintenance Precautions on Semiconductor Units".

When soldering new leads ensure attention to the following:

(a) Use stranded wire for all connections. Stiff wire will cancel the floating action of the connector and will be liable to fracture.

(b) Do not tightly stretch the leads, but leave just sufficient slack to reconnect if the lead should be accidentally broken away.

(c) Do not permit solder to run back along the conductor strands; this spoils the insulant and creates a danger of breakage at some later date.

(d) Programme leads (input and output) should be insulated, screened twin. Expose no more than approximately $\frac{1}{2}$ inch of lead from the screening braid in order to avoid unwanted pick-up. The screening on the output leads should not be finished in a pigtail; trim and cover with a sleeve. The screening on the output signal leads should be earthed at the remote end of the audio cable, NOT to a mains earth.

(e) The screening pigtail of the input leads must go to the signal earth (normally B+ or the B+ busbar). Keep it short and sleeve it to prevent short circuits.

(f) Leads from B+ and B- should not be of smaller gauge than 14/.0076, preferably with thick wall insulation. The heavy gauge is needed in this application because of the low impedance of the power supply. This impedance must not be increased otherwise the stability of the power supply may suffer. For leads longer than 1 yard (1 m) the use of 23/.0076 is strongly advised.

6. DUMMY UNITS AND PANELS

If a frame is being installed then it should be remembered that different sizes of dummy units and back panels are available to fill vacant compartments in the frame. Where forced cooling is present in a rack (or console) these dummy units with their back panels serve not only to ensure a good presentation but also to ensure that the path of the cooling air stream is not diverted in a wasteful manner. On semi-conductor equipments this is of more than normal importance.

7. PARTS LIST

Rack Mounting Frame (19" rack)	749087
Vertical Screen	435629
Horizontal Screen	435630

MAINTENANCE PRECAUTIONS

FOR

SEMICONDUCTOR UNITS

NOTE: Non-observance can lead to destruction of semiconductors.

SECTION 1. GENERAL ELECTRICAL PRECAUTIONS

1.1 CONTINUITY CHECKING

When using any type of meter to check continuity, it is essential to remember that some give a voltage which is sufficient to destroy certain low voltage semiconductors. This is most likely if the polarity of the test voltage is applied incorrectly. Therefore:

(a) Check the polarity of the test meter voltage.
(b) Check the voltage level and see that this is within the rating of the semiconductors.
(c) When checking wiring external to a unit, it is safer to unplug the unit (or units) whenever possible.
When it is required to check resistors, capacitors and other components it must be remembered that if these components are across the whole, or part, of a semiconductor device, the device itself may affect test meter readings. It is necessary in these cases to disconnect one end of the component being checked.
(d) When the potential at the test meter terminals exceeds the semiconductor ratings it will be advisable to disconnect one end of every component which it is necessary to check - but see also 1.2. below.

1.2 SOLDERING

When soldering is undertaken in semiconductor circuits, poor insulation on the iron can give a sufficient level of a.c. leakage to permanently damage semiconductors. It is advisable therefore to make a quick check with a meter between the bit of the iron and the circuit earth. Note: on some units this may not be the chassis. If a potential is present take one of the following steps:

(a) Repair earth on the iron, or get another.
(b) Remove unit's earth by unplugging where possible.
(c) Remove unit's earth by disconnecting temporarily, say at an equipment plug or terminal block.
(d) Fit a switch in the 'live' lead to the iron, and switch off before bit touches the components or wiring.
(e) Use a low voltage iron or one which can be earthed to the equipment (not to the main's earth).

Remember, these precautions also apply when soldering cableform wiring external to the unit.

Never solder with the B+ switched ON. This can lead to disastrous short circuits, e.g. across emitter resistor.

All semiconductors are temperature sensitive, even without the power ON. Therefore;

When soldering use a thermal shunt, e.g. long nosed cool pliers or similar shunt, between the iron and the device.

1.3 VOLTAGE ANALYSIS

When making a voltage analysis be more than normally careful to prevent undesired short circuits by test prods. These can ruin a transistor e.g. if across base and B-, or across emitter resistor. Crocodile clips are a very common cause of accidental short circuits.

1.4 DISCONNECTING SEMICONDUCTOR UNITS

Because high level transients can damage many types of semiconductor always switch off the power supplies before removing the unit or unplugging it. Even if transients are known to be of no importance it is still possible in unplugging to break say a bias line before the B+ and hence give rise to damage.

1.5 TEST POWER SUPPLIES

Where units of an equipment can be unplugged and removed from a rack or console, it is always preferable to use a jumper lead so that the unit may be plugged in to its normal power supply. Check the polarity on the jumper lead (see also 2.5). Where test power supplies must be used observe the following:

(a) Use a power unit with similar characteristics to the one in the equipment e.g. with low ripple, high stabilisation, transient suppression, etc.
(b) Set d.c. supply to nominal ±1V, or better, so that results are meaningful.
(c) Always check polarity before connecting any test supply.
(d) Heavy gauge wire is essential for low impedance B+ supplies, say 23/·0076.

1.6 TEST EQUIPMENT

It should be remembered that items of test equipment often contain capacitors which may be charged as a result of some previous test. This charge may be sufficient to damage semiconductors in the item under test. Therefore:

(a) Always connect test equipment earth wires first to the unit under test, then touch the other connecting lead to earth before connecting it into the unit to be tested.
(b) Observe this kind of precaution with capacitors, whether these are used for test purpose or as replacements, i.e. check that they are discharged.

Signal Generators, especially l.f.types, quite frequently give voltages which far exceed the semiconductor rating. Therefore:

Before connecting this class of instrument into a semiconductor circuit the output should be turned down to minimum and care taken that the output is not subsequently turned up above a safe level.

1.7 SEMICONDUCTOR POWER UNITS

Special components are usual in these units; all are low voltage items. Some are intolerant of overloads. Therefore in all maintenance and servicing operations ensure that incorrect conditions are not introduced e.g. if the mains transformer or its taps have to be changed the connections should be carefully checked to ensure that excess voltage is not applied.

1.8 HIGH VALUE CAPACITORS

High capacity condensers are common on all semiconductor units. Since semiconductor devices are intolerant of large transients, be careful not to charge or discharge high value capacitors through them, e.g. by short circuits when power has been recently applied, or by replacing a capacitor when the B+ is on.

Never discharge the many thousand µF condensers by short circuits in the unit.

1.9 EARTHING

On no account should the earthing system of multi-unit audio installations, video installations, or any others be altered. On transistorised equipment this is more than normally important due to the use of low impedance supplies and the risk of introducing hum and other forms of interference into low signal circuits. The unit circuit earth is not necessarily connected to the mains earth or chassis. Any added B+(earth) wiring should always be in very heavy cable (See 1.5 d.)

This prohibition applies equally to paths for lamp, relay and other similar circuit supplies which are kept separate from signal paths. In this case high ripple (or plain a.c.) voltage may be fed into the signal earth. The resulting earth currents can then be picked up in low level signal circuits and amplified.

1.10 TRANSISTOR TESTING

It is always advisable to use a test item designed specifically for testing semiconductors, since any other item may give misleading results, and may also damage the semiconductor device.

SECTION 2. MECHANICAL PRECAUTIONS

2.1 PAINT

The black paint covering on certain semiconductors is there to stop light from reaching the junction which is sensitive to electromagnetic radiation including regions centred on the frequency of visible light. In fitting and handling, this paint must not be damaged.

2.2 SEMICONDUCTOR LEADS

When replacing, or disconnecting for test, the lead should not be bent closer than 1·5mm with respect to the body since any bending closer than this may damage the seal.

2.3 POWER SEMICONDUCTORS

When replacing power semiconductors the mica insulating washers (if used) must not be damaged; nor may any other material be substituted since this will affect adversely the transfer of heat from the case to the heat sink.

A smear of silicone grease on the washer serves to prevent sticking and also to make a more intimate heat bond to the sink. No other type of grease should be used.

Fixings on power semiconductors should be well tightened since this again affects heat transfer.

With some devices the metal case may be connected to an internal electrode. In these cases care must be taken not to allow the case to touch the chassis, other components, or any nearby tags.

2.4 HEAT SINKS

On no account should the black matt finish be removed from heat sinks (or fins) since this can affect the power handling capacity by an amount varying up to as much as 30% depending on the type of component.

On many small semiconductors a clip is used to increase the power dissipation. Make sure, therefore, that when a device is replaced the same size of clip is used and that this makes close contact with the case.

2.5 FORCED COOLING

Where forced cooling is provided this must not be obstructed since this can affect the power handling capacity by as much as 200% or higher.

When servicing on a test bench, or on jumper leads, the equipment air supply should be simulated or damage may result.

SECTION 3 - STORAGE

3.1 R.F.RADIATION

When units or components are stored this should not be near any high-power r.f. radiation e.g. from transmitters, test installations, etc. Radiation of this type is harmful, especially in the 'S' and 'X-Band'.

3.2 RADIO-ACTIVE EFFECTS

Semiconductors are affected adversely by various radio-active radiations e.g. X-rays, gamma rays and neutrons. Keep them away from any quantity of radio-active valves e.g. T.R.cells and some gas tubes since these contain radio-active materials.

3.3 TEMPERATURE

Although temperature ranges for semiconductors are continually increasing it is still good practice to keep all stocks away from hot radiators etc. and equally, not to permit stocks to accidentally reach very low temperature conditions.

3.4 MAGNETS

Semiconductors should not be stored close to very strong magnets. There is no permanent effect on the semi-conductor material, but part of the device, i.e. the case, may become permanently magnetised and the field from this will then change the performance of the semi-conductor.

This page is blank to preserve page binding order on printing

APPENDIX

DE-MAGNETISATION OF HIGH PERMEABILITY CORES

1. GENERAL

The long term effects arising from the physical maltreatment of Mumetal and other high permeability materials are widely known. Effects which arise as a result of high d.c. current when applied in associated windings either continuously or in surges are not so well known. Increasing use of high permeability materials in transformers, record/playback heads, and other wound assemblies, coupled with the steady increase in remanence figures as new materials become available, make the need for care in one-time simple checking operations more than ever necessary. Fortunately, the precaution to be taken normally only applies when some fault has developed, and it is necessary to check such things as continuity and / or resistance in part of a circuit that includes transformers which have not been designed to carry d.c. current.

2. PRECAUTIONS

It is sometimes forgotten that simple d.c. operated instruments, such as Avometers when used on their resistance ranges for continuity or resistance checks can give quite high ampere-turn figures in the windings which they are used to check. In small modern transformers (and similar components) any such developed field strength has a small, compact mass of core material on which to act. When this small mass is composed of material with characteristics such as high permeability, fairly high remanence, and rather low magnetising force, the effect of the field can be quite marked. The effect shows itself in the overall component as a change of inductance. This will in turn affect the frequency response. The duration of the effect will depend upon a variety of factors but the really important point to remember is that in many cases only if corrective treatment is applied can the effect be cancelled. Therefore a simple rule should be observed that if:

(a) the unit's transformers are small,

(b) the circuit diagram shows that no d.c. flows in the windings,

then no d.c. operated device should be used for checking either continuity or resistance in the purely a.c. items. On such components as physically small output transformers it is normally sufficient to ensure that any d.c. current from test equipment does not exceed the current normally carried by the component.

3. CORRECTIVE TREATMENT

Since accidents are always possible a simple guide to demagnetising is set out in this section. It must be emphasised that since it is often impossible to gauge the extent of the damage caused by electrical maltreatment of wound components no guarantee of correction is implied by the provision of this information.

3.1 SUPPLIES

Normally any 50 c/s or 60 c/s supply is satisfactory. The r.m.s. demagnetising voltage is given in the maintenance section of unit manuals. Current rating of the supply is unlikely to present any problem. For most small input transformers in Audio units a range of a few hundred milliamps is sufficient. For large items a quick calculation based on the a.c. voltage plus the inductance quoted will provide the answer.

Whatever the source of a.c. voltage the waveform should be reasonably sinusoidal and free from harmonics and spikes. It should be remembered that highly inductive voltage regulators often provide a very poor waveform. Quality of the waveform is important since this will have a very considerable effect on the efficiency of the treatment.

3.2 METHOD

The procedure to be followed is set out below.

(a) Connect in series across the a.c. source a limiting resistor, and the full winding of a potentiometer of about 1000 ohms.

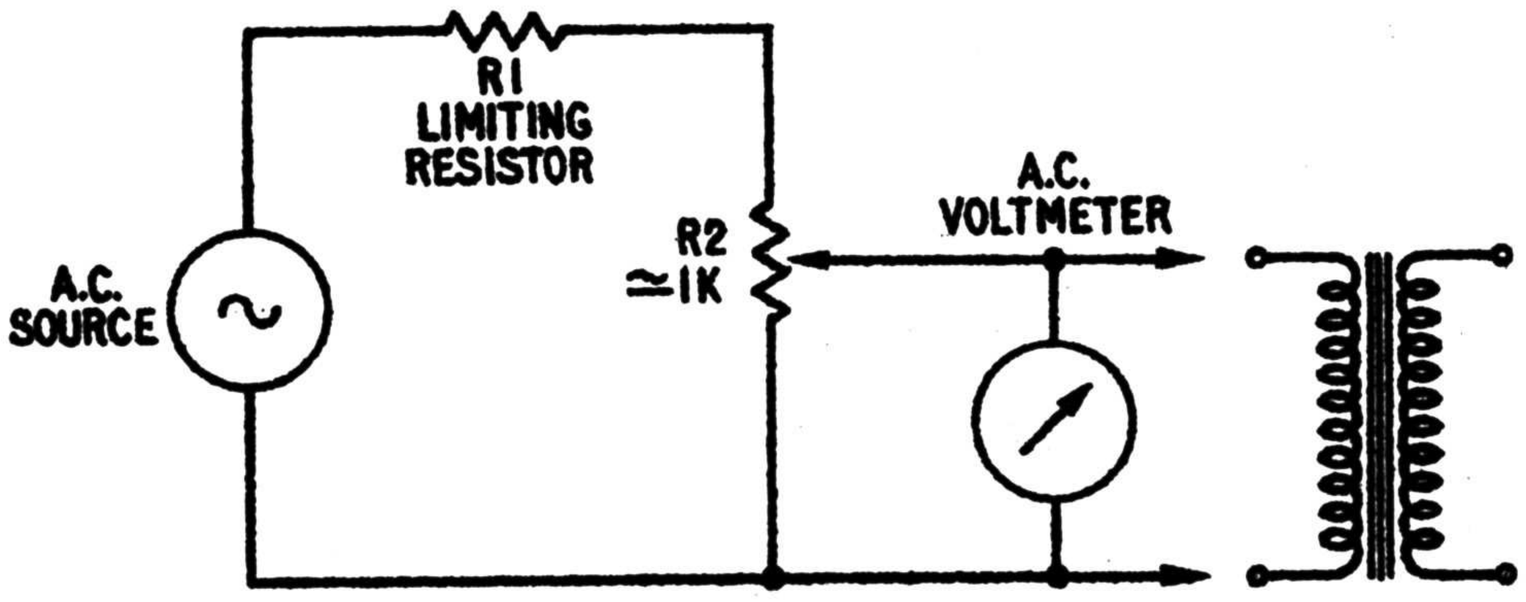


FIGURE 1

(b) Connect the component to be treated and an a.c. voltmeter across the slider of the potentiometer and its contact which is returned to the a.c. supply. Set the potentiometer to give zero volts to the component. (See Figure 1)

NOTE: If Avometers (or similar instruments) are used with a poor waveform the calibration will be in error and allowance must be made in accordance with the handbook supplied by the meter manufacturer.

(c) Switch on the a.c. supply and adjust the potentiometer to give the maximum r.m.s. voltage as shown in the unit manual.

NOTE: The limiting resistor in Figure 1 should be of such a value that if the slider of R1 should accidently be taken to the fullest extent of its travel, the voltage applied to the transformer will be only slightly in excess of the maximum specified.

(d) The voltage should now be gradually reduced to zero in about one minute, but note that the method of doing so is very important. As a rough guide it should be reduced so that a plot of voltage against time would give the well known exponential curve as of a condenser discharging through a fixed resistor. The point to remember is that the longest time is to be spent at the lowest voltages.

(e) If the waveform of the supply contains harmonics (or other departures from a true sine wave) the procedure may have to be repeated a few times.

This page is blank to preserve page binding order on printing

TREATMENT FOR ELECTRIC SHOCK


Human beings are rarely killed outright by electric shock and can, in most cases, be saved by immediate commencement of artificial respiration. Electric shock affects the nerves controlling the breathing and the action of the heart and unless prompt aid is given the victim may become unconscious and die. ALWAYS SEND FOR BUT NEVER WAIT FOR A DOCTOR.

Before touching the injured person, make sure that he is not in contact with a live conductor. If he is, break the circuit by opening the power switch - DO NOT TOUCH THE VICTIM WITH YOUR BARE HANDS. If it is not possible to switch off the current, use a piece of dry insulating material, such as wood, bakelite or rubber, to knock or push aside the conductor. Alternatively, pull the victim free using a leather belt or braces, protecting yourself still further by standing on a folded newspaper or a dry mackintosh.

HOLGER NIELSON METHOD OF ARTIFICIAL RESPIRATION


(1) Immediately the patient is released from electrical contact loosen his collar and any tight clothing as quickly as possible.

(2) Remove false teeth and sweets etc. from the patient's mouth and make sure that the tongue is free by giving two or three firm slaps with the flat of the hand between the shoulder blades.

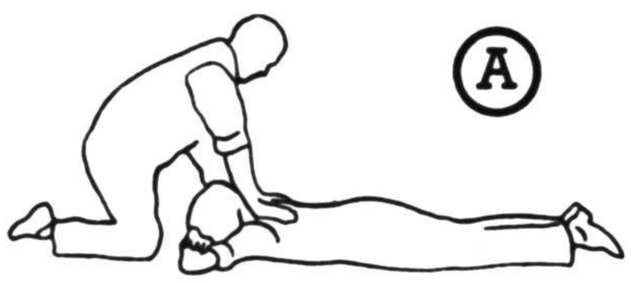

(3) Lay the patient face downwards with the forehead resting on the fore arms so that the mouth and nose are kept clear of the ground (A).

(4) Kneel on one knee a little in front of and to the side of the patient's head so that the left foot is at the side of the patient's elbow. (A). The arms should slope forward so that the hands lie close together on the patient's shoulders with the wrists over the top of the shoulder blades. This is the starting position.

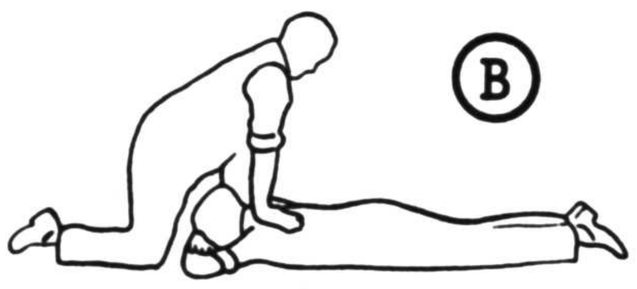


(i) Rock forward on outstretched arms until the arms are vertical above the patient's body (B). The pressure should be light and without force; the movement should take approximately 2 seconds.

(ii) Release the pressure by allowing the hands to slide quickly down the patient's arms to the elbows taking approximately $\frac{1}{2}$ a second (C). Then raise his arms and shoulders slightly, at the same time moving your body backwards (D), taking approximately 2 seconds.



(iii) Lower the patient's arms until they touch the ground (E), and return your hands to the original position on his shoulders and resume the position as before. Take approximately $\frac{1}{2}$ a second for this movement.

(5) Repeat the movements described in (i), (ii) and (iii) so that the complete cycle takes approximately six seconds. That is, about nine complete respirations per minute.

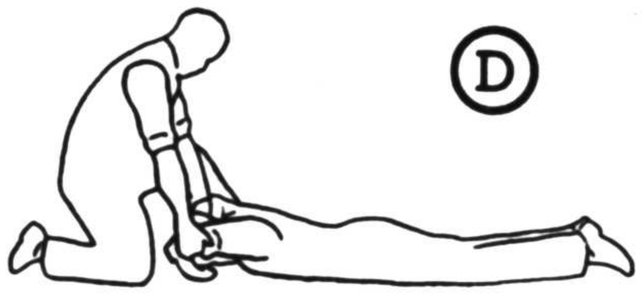

(6) Whilst artificial respiration is continued have someone else:-

(a) Loosen patient's clothing and keep him warm.


(b) Send for a doctor.

(c) Watch so that they can take over if prolonged treatment is necessary.

(7) Keep going for at least four hours even if there is no sign of recovery.

(8) Do not move the patient until he is breathing normally without assistance. There should be no hurry to move him after he has recovered.

(9) Do not give the patient oxygen or other stimulants unless ordered to by a doctor. When fully recovered the patient may be allowed to drink cold water with, if available, one teaspoonful of Sal Volatile to a glass. He may also be permitted to sniff smelling salts.

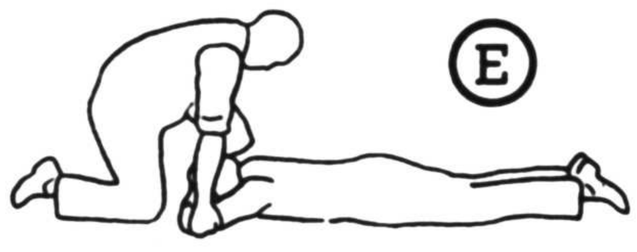

TREATMENT FOR BURNS

If as a result of electric shock the patient is suffering from burns, the following treatment should be given without hindrance to artificial respiration:-

(1) Remove the clothing near the affected part to enable the burn/s to be treated, taking care not to break any blisters that may have formed.

(2) Saturate the burn/s using a warm solution made up of one desertspoonful of bi-carbonate of soda and a pint of warm water. If bi-carbonate of soda is not available, use a teaspoonful of salt.

(3) Cover the burns with lint soaked in the above solution and apply a bandage taking care not to burst any blisters that may have formed.

(4) If a solution as above is not available cover the burns with a sterile dressing to exclude the air.